

Mouse (ALT) ELISA Kit



Catalog Number: EK18815

This kit allows for the determination of ALT concentrations in Mouse serum, plasma, tissue homogenates and other biological fluids.

This instruction must be read in its entirety before using this product.

For research use only. Not for use in diagnostic procedures.

Contact information

Tel: 1-301-446-2499

Fax: 1-301-446-2413

Email: tech@signalwayantibody.com

Web: www.sabbiotech.com

Assay range: 2ng/L -90ng/L

Principle of the assay

The kit assay Mouse ALT level in the sample, use Purified Mouse ALT antibody to coat microtiter plate wells, make solid-phase antibody, then add ALT to wells, Combined ALT antibody which With HRP labeled , become antibody - antigen - enzyme-antibody complex, after washing Completely, Add TMB substrate solution, TMB substrate becomes blue color At HRP enzyme-catalyzed, reaction is terminated by the addition of a sulphuric acid solution and the color change is measured spectrophotometrically at a wavelength of 450 nm. The concentration of Mouse ALT in the samples is then determined by comparing the O.D. of the samples to the standard curve.

Materials provided with the kit

1	Wash solution	20ml×1bottle	7	Stop Solution	3ml×1 bottle
2	HRP-Conjugate reagent	3ml×1 bottle	8	Standard (160ng/L)	0.5ml×1 bottle
3	Microelisa stripplate	12well×4strips	9	Standard diluent	1.5ml×1bottle
4	Sample diluent	3ml×1 bottle	10	Instruction	1
5	Chromogen Solution A	3ml×1 bottle	11	Closure plate membrane	8
6	Chromogen Solution B	3ml×1 bottle			

Specimen requirements

1. extract as soon as possible after Specimen collection, and according to the relevant literature, and should be experiment as soon as possible after the extraction. If it can't, specimen can be kept in -20 °C to preserve, Avoid repeated freeze-thaw cycles.
2. Can't detect the sample which contain NaN₃, because NaN₃ inhibits HRP active.

Assay procedure


1. Dilute and add sample: Dilute Original density Standard as follow table:

80ng/L	5 Standard	150 μ l Original density Standard+150 μ l Standard diluent
40ng/L	4 Standard	150 μ l 5 Standard+150 μ l Standard diluent
20ng/L	3 Standard	150 μ l 4 Standard+150 μ l Standard diluent
10ng/L	2 Standard	150 μ l 3 Standard +150 μ l Standard diluent
5ng/L	1 Standard	150 μ l 2 Standard +150 μ l Standard diluent

2. add sample: Set blank wells separately (blank comparison wells don't add sample and HRP-Conjugate reagent, other each step operation is same). testing sample well. add standard 50 μ l in the Microelisa stripplate accurately, add Sample dilution 40 μ l to testing sample well, then add testing sample 10 μ l (sample final dilution is 5-fold), add sample to wells, don't touch the well wall as far as possible, and Gently mix.
3. Incubate: After closing plate with Closure plate membrane ,incubate for 30 min at 37°C.

4. Configure liquid: 30-fold(or 20-fold) wash solution diluted 30-fold (or 20-fold) with distilled water and reserve.
5. washing: Uncover Closure plate membrane, discard Liquid, dry by swing, add washing buffer to every well, still for 30s then drain, repeat 5 times, dry by pat.
6. add enzyme: Add HRP-Conjugate reagent 50 μ l to each well, except blank well.
7. incubate: Operation with 3.
8. washing: Operation with 5.
9. color: Add Chromogen Solution A 50ul and Chromogen Solution B to each well, evade the light preservation for 10 min at 37 $^{\circ}$ C
10. Stop the reaction: Add Stop Solution50 μ l to each well, Stop the reaction(the blue color change to yellow color).
11. assay: take blank well as zero , Read absorbance at 450nm after Adding Stop Solution and within 15min.

Steps description

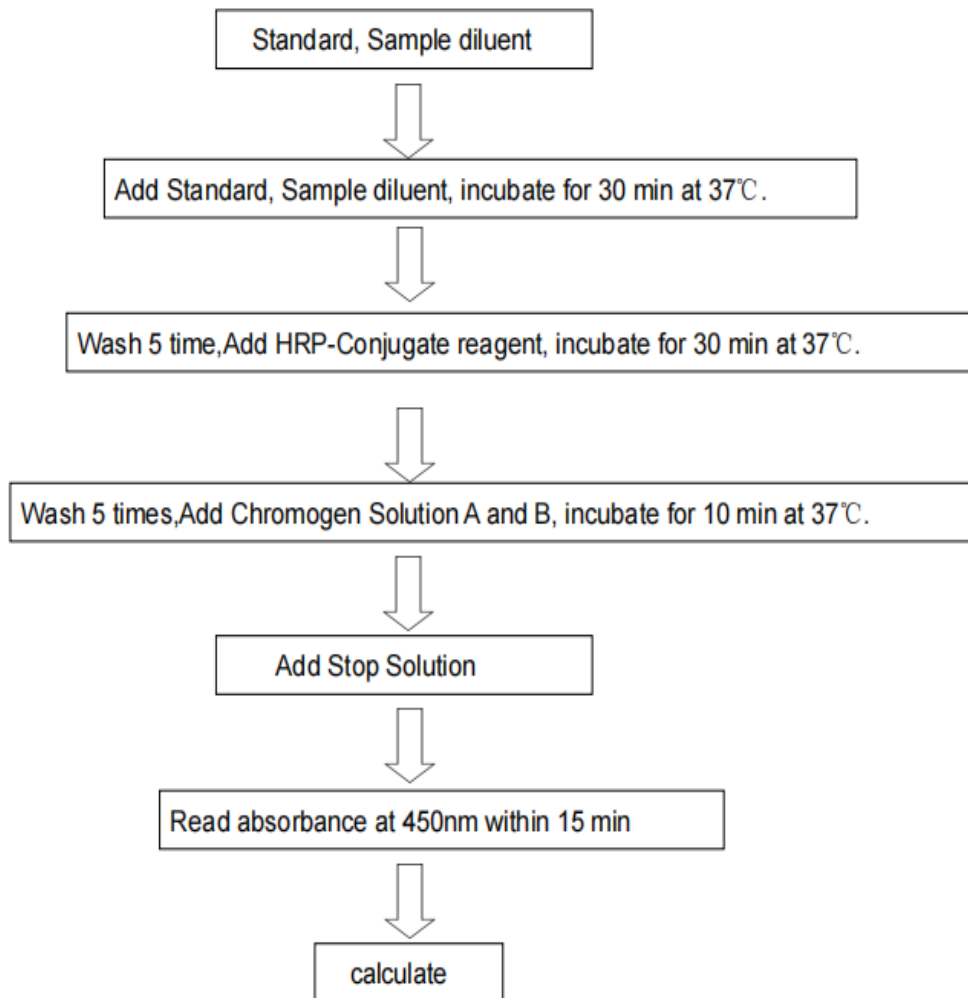

Calculate

Take the standard density as the horizontal, the OD value for the vertical, draw the standard curve on graph paper, Find out the corresponding density according to the sample OD value by the Sample curve, multiplied by the dilution multiple, or calculate the straight line regression equation of the standard curve with the standard density and the OD value, with the sample OD value in the equation, calculate the sample density, multiplied by the dilution factor, the result is the sample actual density.

Important notes

1. The kit takes out from the refrigeration environment should be balanced 1 hour in the room temperature, ELISA plates coated if has not use up after opened, the plate should be stored in Sealed bag.
2. washing buffer will Crystallization separation, it can be heated the water helps dissolve when dilute . Washing does not affect the result.
3. add Sample with sampler Each step, And proofread its accuracy frequently, avoids the experimental error. add sample within 5 min, if the number of sample is much , recommend to use Volley .

4. if the testing material content is excessively higher (The sample OD is bigger than the first standard well),please dilute Sample (n-fold), Please diluente and multiplied by the dilution factor. ($\times n \times 5$) .
5. Closure plate membrane only limits the disposable use, to avoid cross-contamination.
6. The substrate evade the light preservation.
7. Please according to use instruction strictly, The test result determination must take the microtiter plate reader as a standard.
8. All samples, washing buffer and each kind of reject should according to infective material process.
9. Do not mix reagents with those from other lots.

Storage and validity

1. Storage: 2-8°C.
2. validity: six months